

CELIAC REAL-TIME PCR KIT (HLA-DQ2, HLA-DQ8)

Cat. No: 111R-20-04

INTRODUCTION

Celiac disease is a genetically determined immune-mediated disorder, that develops in genetically susceptible individuals mainly as a result of enteric exposure to gluten proteins after digestion of wheat, barley and rye. The genetic risk factors for celiac disease have been well characterized. More than 90% of the patients carry a major histocompatibility complex class II human leukocyte antigen (HLA) variant called DQ2 (encoded by DQB1*02 and DQA1*05). Most of the remainder carry an HLA variant called DQ8 (encoded by DQB1*0302 and DQA1*03). DQ2 and DQ8 variants are necessary for the development of celiac disease ⁽¹⁾.

INTENDED USE

Celiac Real-Time PCR Kit (HLA-DQ2, HLA-DQ8) can detect HLA-DQ2 (encoded by DQB1*02 and DQA1*05) and HLA-DQ8 (encoded by DQB1*0302 and DQA1*03) variants.

TARGETED USER

For professional use only. Testing should be performed by professionals trained in molecular techniques.

PRINCIPLE OF THE SYSTEM

During the PCR reaction, the DNA polymerase cleaves the probe at the 5' end and separates the reporter dye from the quencher dye only when the probe hybridizes perfectly to the target DNA. This cleavage results in the fluorescent signal which is monitored by Real-Time PCR detection system. An increase in the fluorescent signal (C_T) is proportional to the amount of the specific PCR product ^(2,3).

PRODUCT SPECIFICATION

Each isolated DNA should be tested with two master mixes separately. The kit provides reagents in a "ready-to-use" master mix format which has been specifically adapted to 5' nuclease PCR for SNP analysis. The test system is designed by SNP Biotechnology for use with sequence specific primers and probes.

The fluorescence of HLA-DQ2-DQ8 variants are FAM and Texas Red. Also each master mix contains an internal control labelled with HEX/JOE dye (See Table 2). Internal Control is Prothrombin gene – FII (OMIM: 176930). The limit of detection (LOD) for the Celiac Real-Time PCR Kit (HLA-DQ2, HLA-DQ8) was determined as 1 ng/ μ l.

SYSTEM CONTENTS

Reagents	10 rxns	20 rxns	50 rxns
Celiac Mix 1	200 μ l	400 μ l	1000 μ l
Celiac Mix 2	200 μ l	400 μ l	1000 μ l
Control DNA*	30 μ l	30 μ l	60 μ l

Table 1: Kit content

* Control DNA is a synthetic plasmid containing the HLA-DQ2 and HLA-DQ8 variants indicated on the tube label. Since to Control DNA is a synthetic plasmid, amplification plots of synthetic control DNA may appear slightly different from the sample DNA. Please gently vortex and then spin centrifuge for 1-2 seconds before use the positive control.

STORAGE

- All reagents should be stored at – 20 °C and dark.
- All reagents can be used until the expiration date on the box label.
- Repeated thawing and freezing (>4X) should be avoided, as this may reduce the sensitivity of the assay.

SAMPLE COLLECTION

Celiac Real-Time PCR Kit (HLA-DQ2, HLA-DQ8) is approved for use with whole blood samples.

- Standard precautionary instructions must be followed by all healthcare professionals during the collection and transportation of whole blood samples.
- Whole blood samples should be collected in appropriate containers before delivery to the laboratory.
- Freezing and thawing of samples should be avoided.

DNA EXTRACTION

Blood samples should be collected in appropriate sterile EDTA tubes and can be stored at +4°C up to one month. For more than one month specimen should be stored at -20°C. It is advised to gently mix the tube (with EDTA) after collection of blood to avoid coagulation.

Our system optimized according to GeneAII® Exgene™ Blood SV. It is advised to elute DNA with 150 μ l elution buffer for better results.

VARIANTS / DYE TABLE

Tubes	Variants	Dyes
Mix 1	DQB1*02	FAM
	DQA1*05	Texas Red
	Internal Control	HEX/JOE
Mix 2	DQB1*0302	FAM
	DQA1*03	Texas Red
	Internal Control	HEX/JOE

Table 2: Tubes - variants - dyes.

PROCEDURE

- Different test tubes should be prepared for each master mix.
- Leave the master mixes* and controls at RT to melt.
- Before starting work, mix the master mixes gently by pipetting
- For each sample, pipet **20 μ l master mix** with micropipets of sterile filter tips to each optical white strips or tubes.
- Add **5 μ l DNA** into each tube. Please do not pipette DNA before and after addition into well.
- Optical caps are closed, it is recommended to spin the plates/strips at low speed for a short time.
- Run with the programme shown below.

*Master mixes include HotStart Taq DNA Polymerase.

PCR PROGRAMME

95 °C	3 Min.	Holding
95 °C	15 Sec.	30 Cycles
60 °C	1 Min.	

Table 3: PCR Programme

Fluorescent dyes are FAM, HEX/JOE and Texas Red.

This system can be used with the following devices:

- Bio-Rad CFX96, Opus 96
- ABI Prism® 7500/7500 Fast
- Mic qPCR Cycler

For other four or more channel Real-Time PCR devices (which can read FAM, HEX/JOE and Texas Red), a trial run is recommended.

If you use:

ABI Prism® system, please choose "none" as passive reference and quencher.

Mic qPCR Cycler, please adjust gain settings, "Green Auto Gain" to 20 and "Yellow Auto Gain" to 10

Supplied Materials

- White PCR plates/strips with optical covers*

*The PCR Plate/strip tube and caps seriously affect the amplification curve quality. Therefore, white PCR plates/strips and optical caps provided by the manufacturer should be used with the kit.

Required Materials (Not Provided)

- PCR Cabinet
- Vortex Mixer
- Desktop Microcentrifuge (For 2.0ml tubes and PCR strip tubes), plate spin for studies using PCR plates.
- Automated or spin column based DNA isolation Kit
- Disposable powder-free laboratory gloves
- Micropipettes (0.5ml-1000ml)
- Micropipette tips
- Standard laboratory equipments.

DATA ANALYSIS

After the run is completed data are analysed using the software with FAM, HEX/JOE and Texas Red. The below results were studied with Bio-Rad CFX96. The threshold values for all dyes were set to 500, based on experiments conducted using the Bio-Rad CFX96 Real-Time PCR system, the GeneAll® Exgene™ Blood SV Isolation Kit, and white PCR strips supplied by SNP Biotechnology. Threshold values may vary depending on the PCR device, DNA isolation kit, and the type or brand of PCR strips/tubes used.

Internal control amplification plots must be seen in all wells except NTC and has been labelled with HEX/JOE dye. The C_T value of internal controls should be $21 \leq C_T \leq 27$ (Figure 1). These values are optimised according to the GeneAll® Exgene™ Blood SV Isolation Kit and Bio-Rad CFX96 Real-Time PCR Device. C_T values may vary $\pm 2/3$ cycle according to the other DNA isolation systems and Real-Time PCR devices.

Amplification plots of HLA-DQ2 and HLA-DQ8 variants can be analysed by FAM and /or Texas Red dyes (Figure 2-5). The C_T value should be between $21 \leq C_T \leq 27$ for positive sample. These values are optimised according to the GeneAll® Exgene™ Blood SV Isolation Kit and Bio-Rad CFX96 Real-Time PCR Device. C_T values may vary $\pm 2/3$ cycle according to the other DNA isolation systems and Real-Time PCR devices.

If there is amplification in the FAM and/or Texas Red dye, the sample is positive for related variant (see Table 2). If there is no amplification in these dyes, the sample is considered negative (Figure 6).

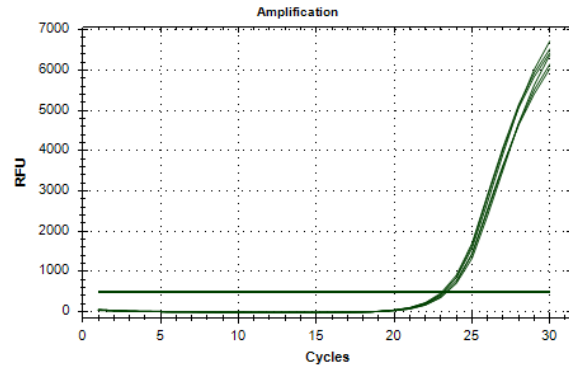


Figure 1: Internal Control plots – HEX/JOE Dye

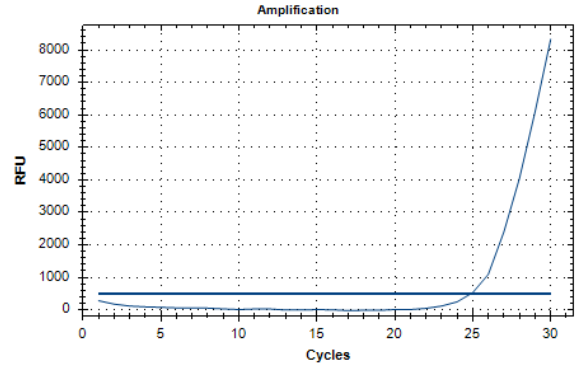


Figure 2: DQB1*02 Positive Sample (FAM Dye – Mix 1)

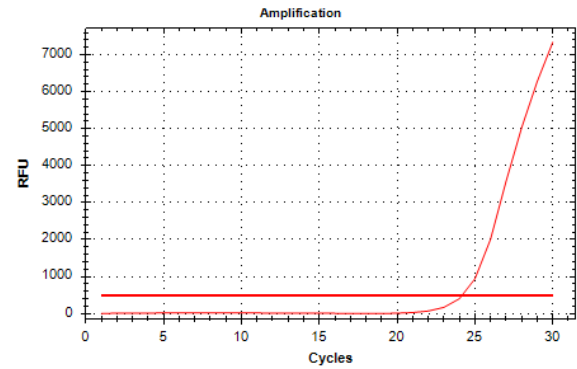


Figure 3: DQA1*05 Positive Sample (Texas Red Dye – Mix 1)

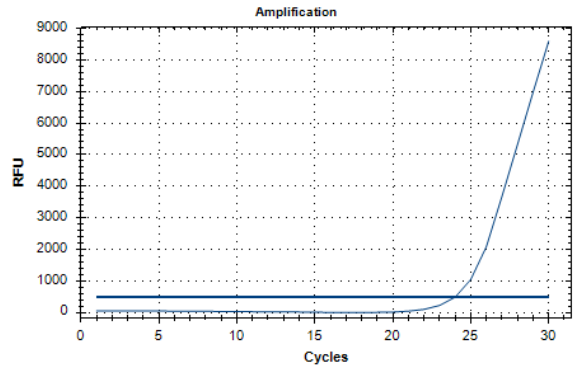


Figure 4: DQB1*0302 Positive Sample (FAM Dye – Mix 2)

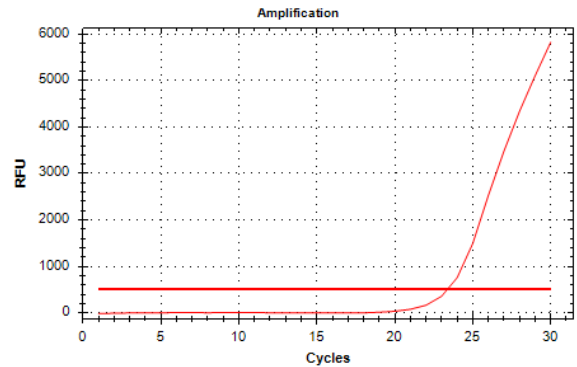


Figure 5: DQA1*03 Positive Sample (Texas Red Dye – Mix 2)

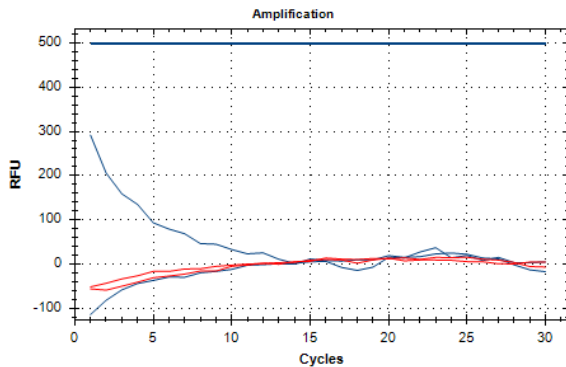


Figure 6: HLA-DQ2 – HLA-DQ8 Negative Sample (FAM and Texas Red Dyes – Mix 1 and Mix 2)

CAUTIONS

- All reagents should be stored at suitable conditions.
- Do not use the PCR master mixes forgotten at room temperature.
- Thaw PCR master mix at room temperature and slowly mix by inverting before use.
- Shelf-life of PCR master mixes is 12 months. Please check the manufacturing data before use.
- Only use in vitro diagnostics.

DISPOSAL OF KIT

Dispose of it according to the legal regulations of your region

LIMITATION OF KIT

In rare cases, B1*0302 primers give non-specific amplification with the B1*0305 subtype. Because the frequency of the B1*0305 allele and its association with the disease are so rare, this condition is ignored. Allele distributions can be viewed at the link: <http://pypop.org/popdata/2008/byfreq-DQ.php.html>

TROUBLESHOOTING PROBLEMS AND SOLUTIONS

Problem	Reason	Solution
Internal control does not work/ low amplification	Absence of DNA / DNA extraction problems	Repeat test
	Absence of DNA / DNA extraction problems	• DNA extraction should be repeated.
	Sample is containing PCR inhibitor(s)	• DNA extraction should be replaced with one of the recommended methods.
No target DNA/internal control amplification curves in all wells	Error in temperature/time settings in PCR program	Correct any errors in the temperature/time settings in the PCR Program and repeat the test.
	Sample is containing PCR inhibitor(s)	• DNA extraction should be repeated. • DNA extraction should be replaced with one of the recommended methods.
Positive control result and/or C_T values are lower or higher than the value mentioned in User Manual.	Error in temperature/time settings in PCR program	Correct any errors in the temperature/time settings in the PCR Program and repeat the test.
C_T values are not valid (higher or lower) according to User Manual	Excessive or insufficient DNA sample	• Repeat the test. • DNA extraction should be repeated.
Low and/or invalid amplification curves	Stability problems arising from repeated thawing and freezing (>4X)	Repeated thawing and freezing (>4X) should be avoided, as this may reduce the sensitivity of the assay.
	Sample is containing PCR inhibitor(s)	• DNA extraction should be repeated. • DNA extraction should be replaced with one of the recommended methods.
	Stability problems arising from unavailable storage conditions.	All reagents should be stored at – 20 °C and dark.
	Bubble formation or pipetting error during pipetting	After adding the master mix and sample, it is recommended to spin the plates/strips at low speed for a short time.

For further questions, please contact us tech@snp.com.tr

Table 5: Troubleshooting problems and solutions

SYMBOLS AND DESCRIPTIONS

	Catalog Number		CE Mark
	Lot Number		Unique Device Identifier (01)Device Identifier (17)Expiry Date (10)Lot Number
	Manufacturer		Test Quantity
	Fragile		Storage Temperature
	Protect from directly sunlight		In Vitro Diagnostics
	Expiry Date		

Table 4: Symbols and descriptions

REFERENCES

1. Francesca Megiorni and Antonio Pizzuti. "HLA-DQA1 and HLA-DQB1 in Celiac disease predisposition: practical implications of the HLA molecular typing". Journal of Biomedical Science 2012, 19:88.
2. Yolanda S Lie and Christos J Petropoulos. "Advances in quantitative PCR technology: 5' nuclease assays". Current Opinion in Biotechnology Volume 9, Issue 1, February 1998, Pages 43-48.
3. Luis Ugozzoli and R. Bruce Wallace. "Allele-Specific Polymerase Chain Reaction". A Companion to Methods in Enzymology Vol. 2, No. 1, February, pp. 42-48, 1991.